


# SkyLite™

TIPLESS NITINOL STONE BASKET



Engineered for  
enhanced endoscopic  
visibility

# The BARD® SKYLITE™ Tipless Nitinol Stone Basket features a “no tip” basket designed to help with atraumatic retrieval of stones in the ureter and calyces.


## FLEXIBILITY. DURABILITY.

Allows for full 270° deflection of a flexible ureteroscope.

Designed for reliable and durable performance in a fully deflected flexible ureteroscope.

The spring loaded sheath is designed to protect the basket from damage or distortion during stone retrieval.

Constructed of Nitinol, the SKYLITE™ Basket offers a kink-resistant design, to help with stone extraction.

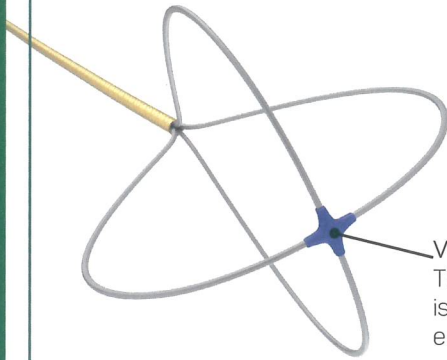

### VisiBLUE™ TECHNOLOGY

The BARD® SKYLITE™ Tipless Nitinol Stone Basket is engineered to enhance visibility under endoscopic light.

Item Number	Sheath (Fr)	Working Length (cm)	Basket Diameter (mm)
041900	1.9	120	12
042400	2.4	120	12
043000	3.0	120	16

**Description:** The BARD® SKYLITE™ Tipless Nitinol Stone Basket consists of a handle to open, close and rotate the basket, a flexible polyimide shaft and a 4-wire nitinol stone basket. The package includes one (1) basket and one (1) introducer.

**Indications for Use:** This device is intended for use in endoscopic removal of ureteral and renal stones.

**Contraindications:** None known

**Warnings:**

- Some objects may be too large to be removed endoscopically using a retrieval device. The use of fluoroscopy and/or x-ray to determine the size of the object is recommended. Do not use the BARD® SKYLITE™ Tipless Nitinol Stone Basket if the object is too large to be removed endoscopically, as it may result in patient injury and pain.
- This is a single use device. Do not resterilize any portion of this device. Reuse and/or repackaging may create a risk of patient or user infection, compromise the structural integrity and/or essential material and design characteristics of the device, which may lead to device failure, and/or may lead to injury, illness or death of a patient.
- Do not attempt to repair, reassemble, or alter the device in any way.
- After use, this product will be a potential biohazard. Handle and dispose of in accordance with accepted medical practices and with applicable laws and regulations. Follow your institutional guidelines.

**Caution:** Objects that are too large to be removed through the scope channel will require the scope and basket to be removed simultaneously

from the urinary tract. If resistance is encountered during advancement or withdrawal of the device, stop and determine the source of resistance, as continued resistance may damage the device and could result in patient injury. Take action to alleviate the resistance.

**Precautions:** Before using, inspect for any breach of packaging to ensure sterility of product. Do not use if breach in sterile barrier is obvious or suspected. Do not allow the device to come in contact with any electrified instruments or laser.

Kinks in the sheath will hinder the mechanical operation of the basket, may affect insertion or withdrawal of the basket and has the potential to damage the endoscope’s instrument channel.

Do not allow the device to be directly fired upon by any lithotripsy devices. To do so may result in damage to the device and could result in patient injury.

Potential complications that may result from the use of a basket in an endoscopic urological procedure include, but are not limited to:

- Perforation · Evulsion · Edema · Entrapment · Laceration · Basket Inversion · Hemorrhage · Inability to disengage from irretrievable object